

Fig 1. Equipment Setup

Proton range QA for 97 energies in 10 minutes with 0.1mm precision

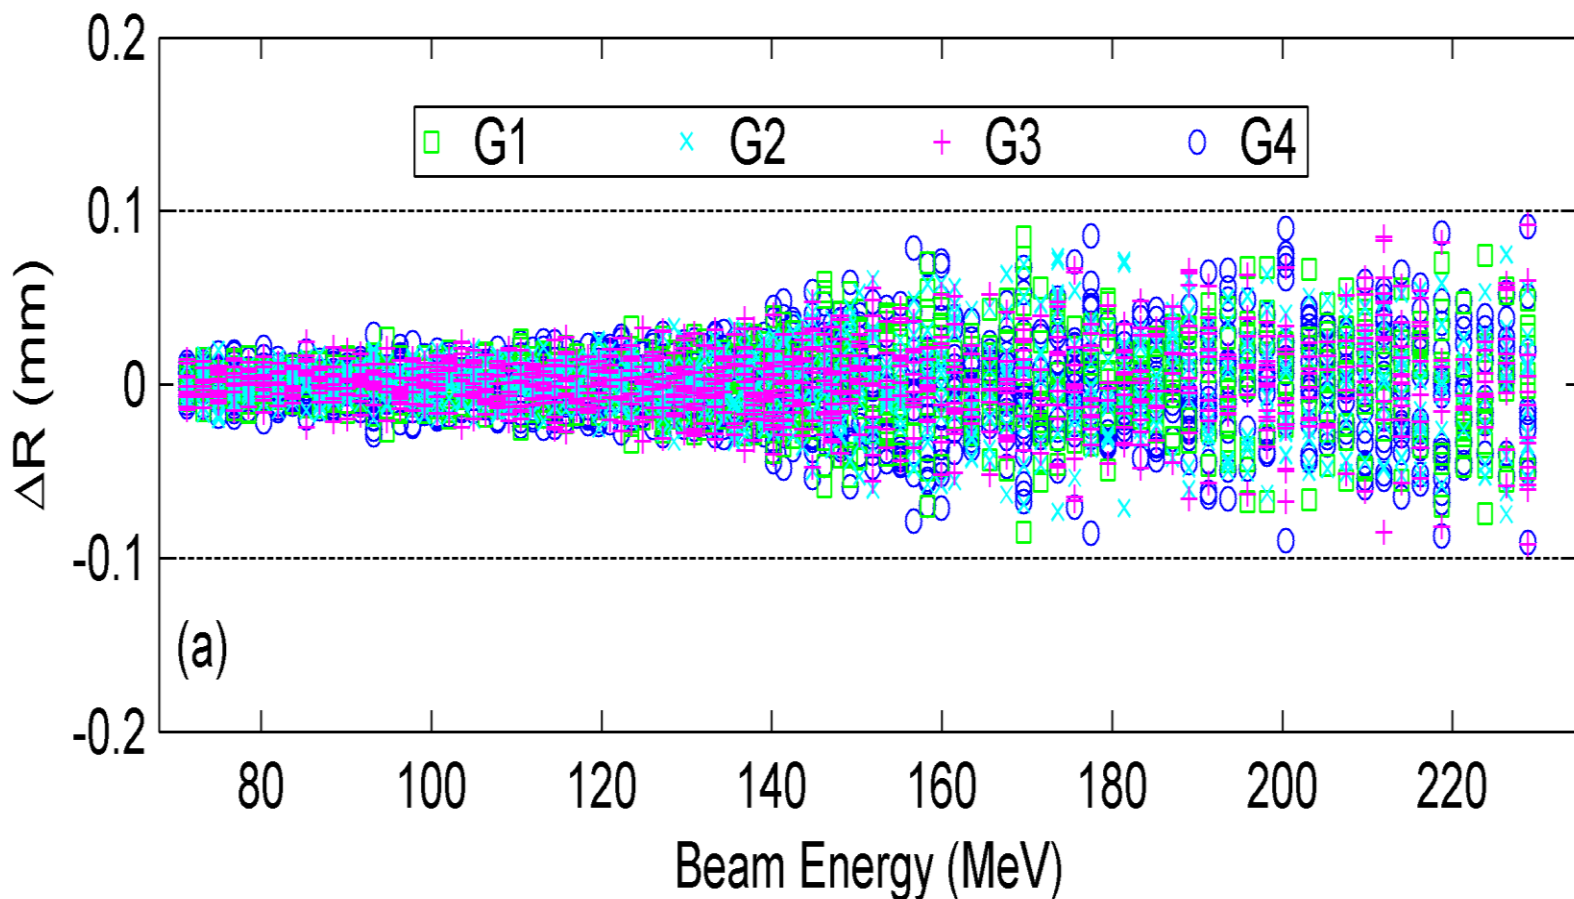


Fig 2. The range reproducibility (ΔR) for all four gantry rooms (G1-G4)

Session: Dose Calculation, Delivery and Measurement Techniques
 Time: 07/31 | 5:40PM, Karl Dean Ballroom C
 Presenting Author: Wei Deng (xiguopi1@gmail.com)
 Corresponding Author: Jiajian Shen (Shen.Jiajian@mayo.edu)